

FIG. 1


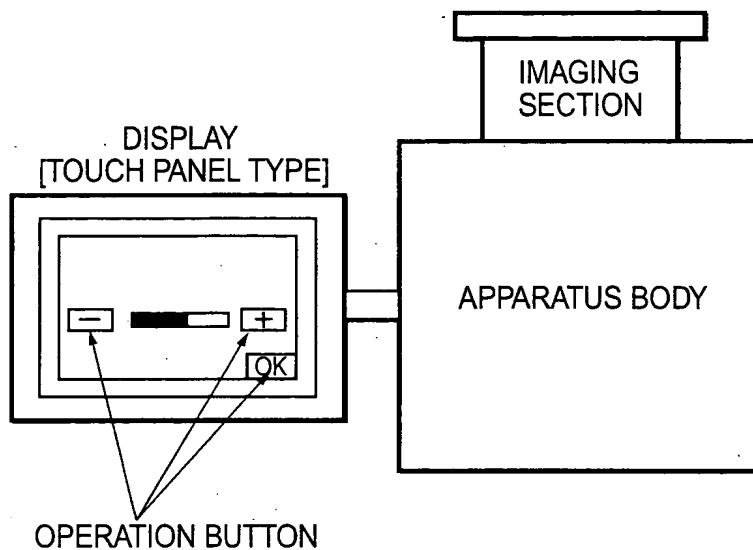


FIG. 2

IMAGING APPARATUS

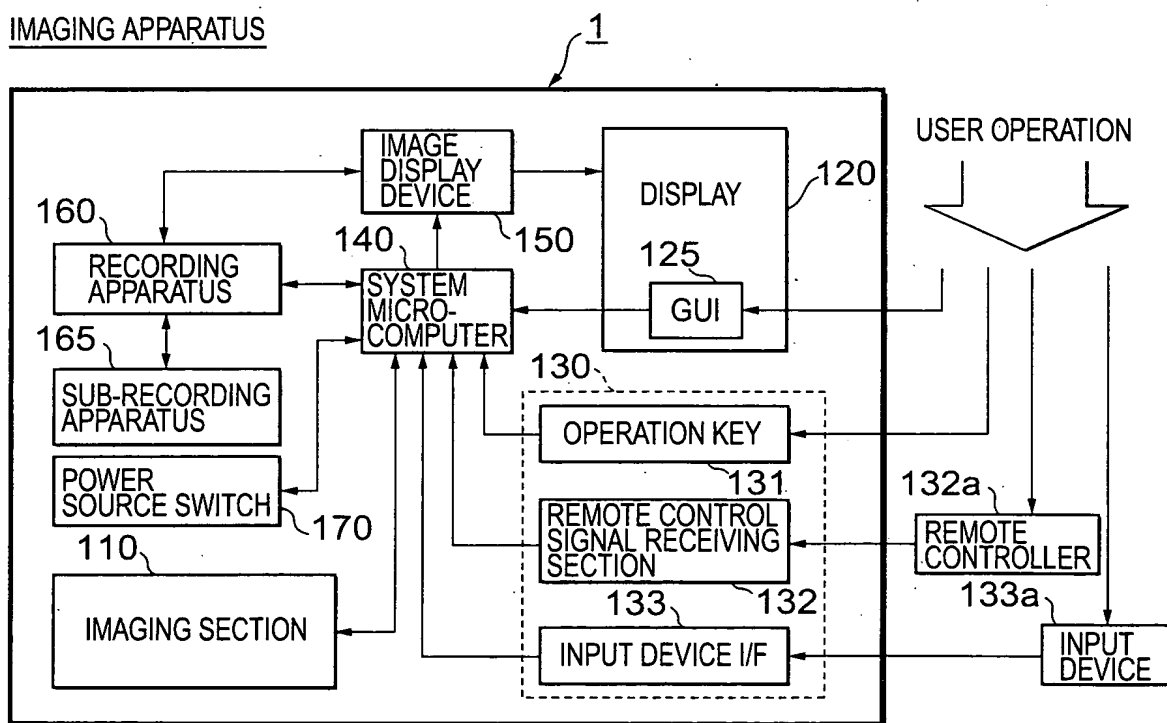

2/25

FIG. 3

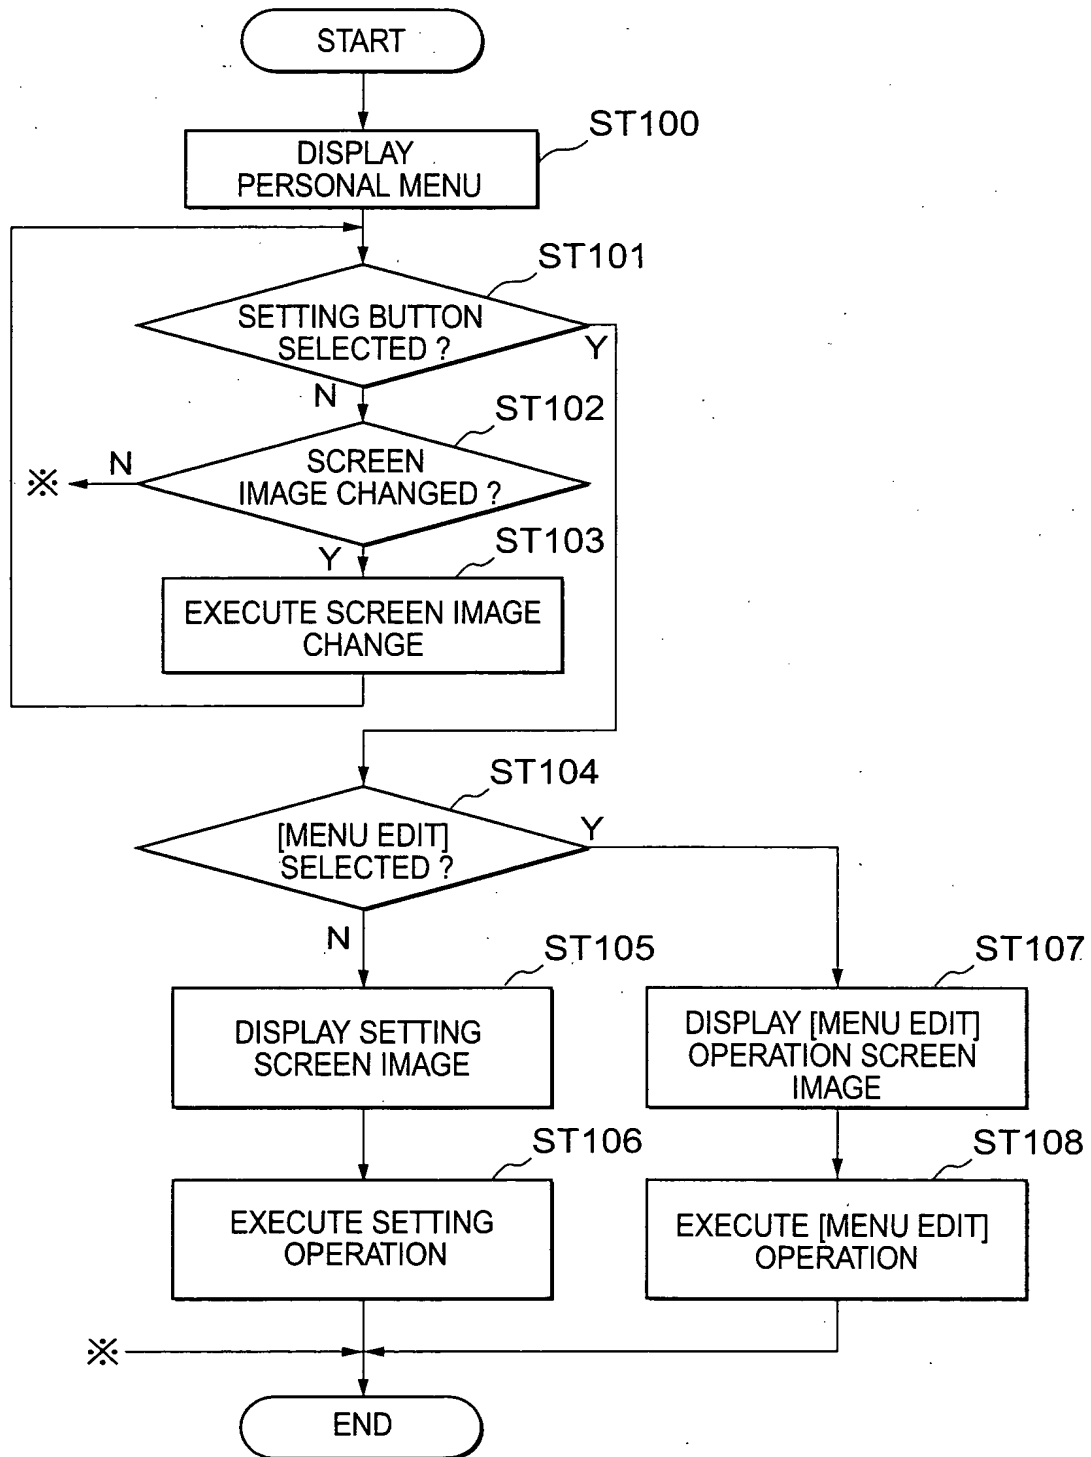


FIG. 4

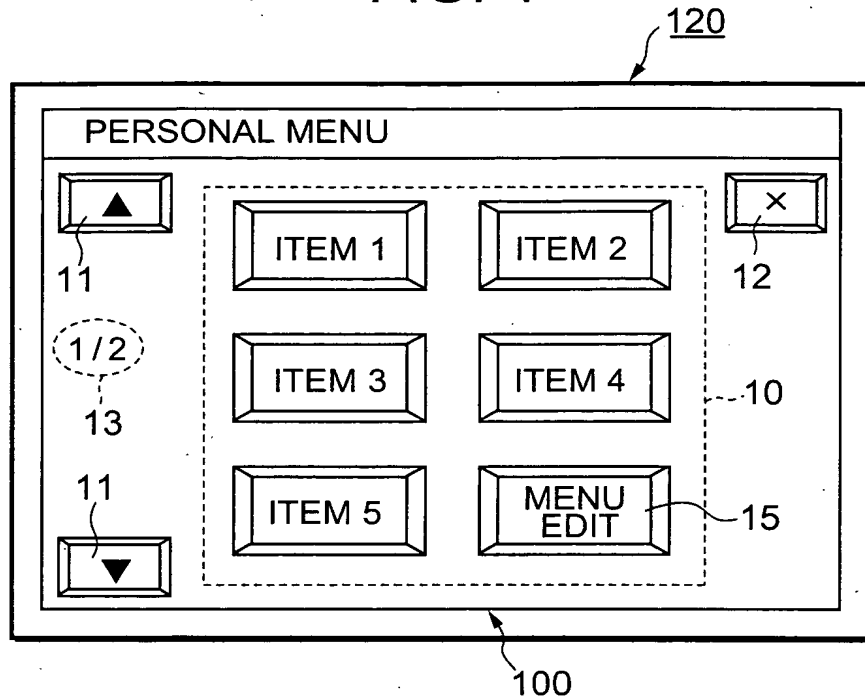


FIG. 5



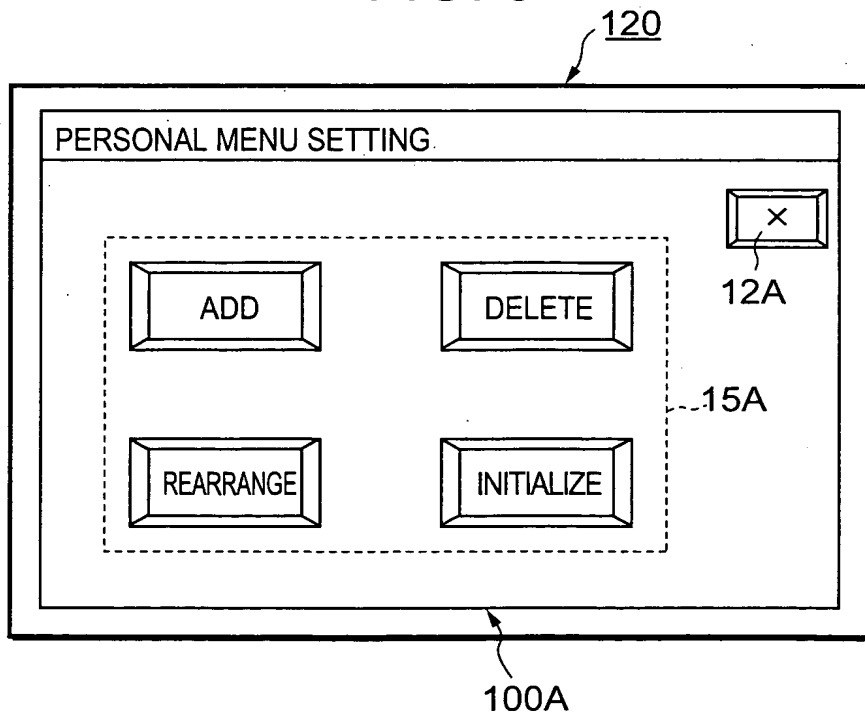


FIG. 6

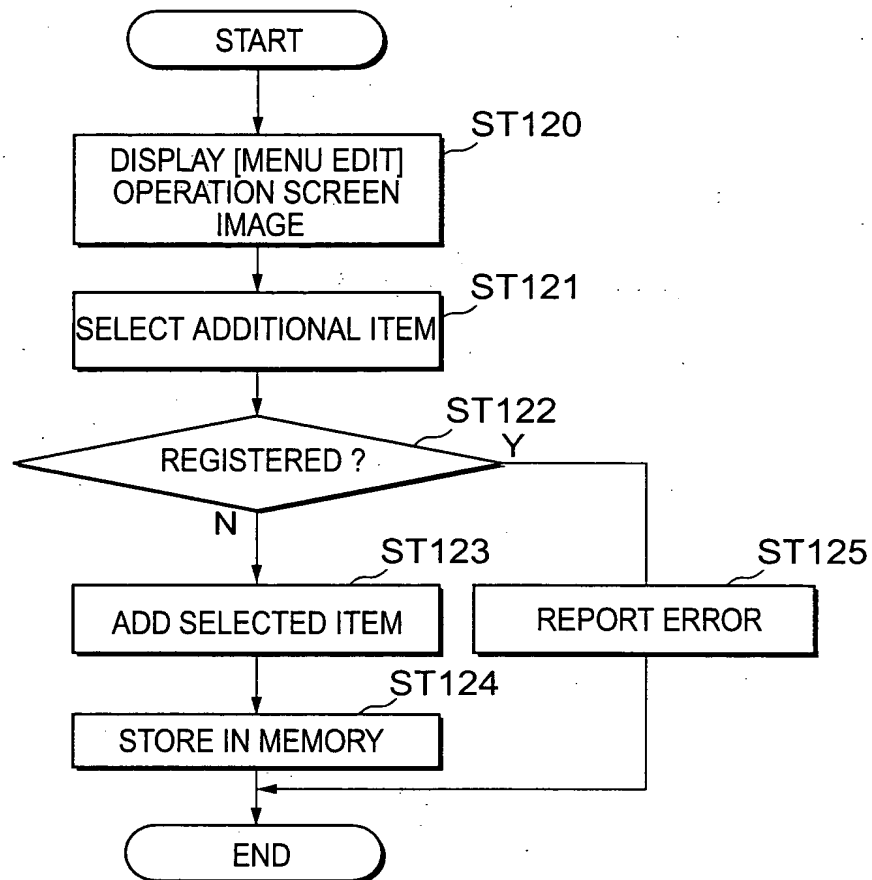


5/25

FIG. 7

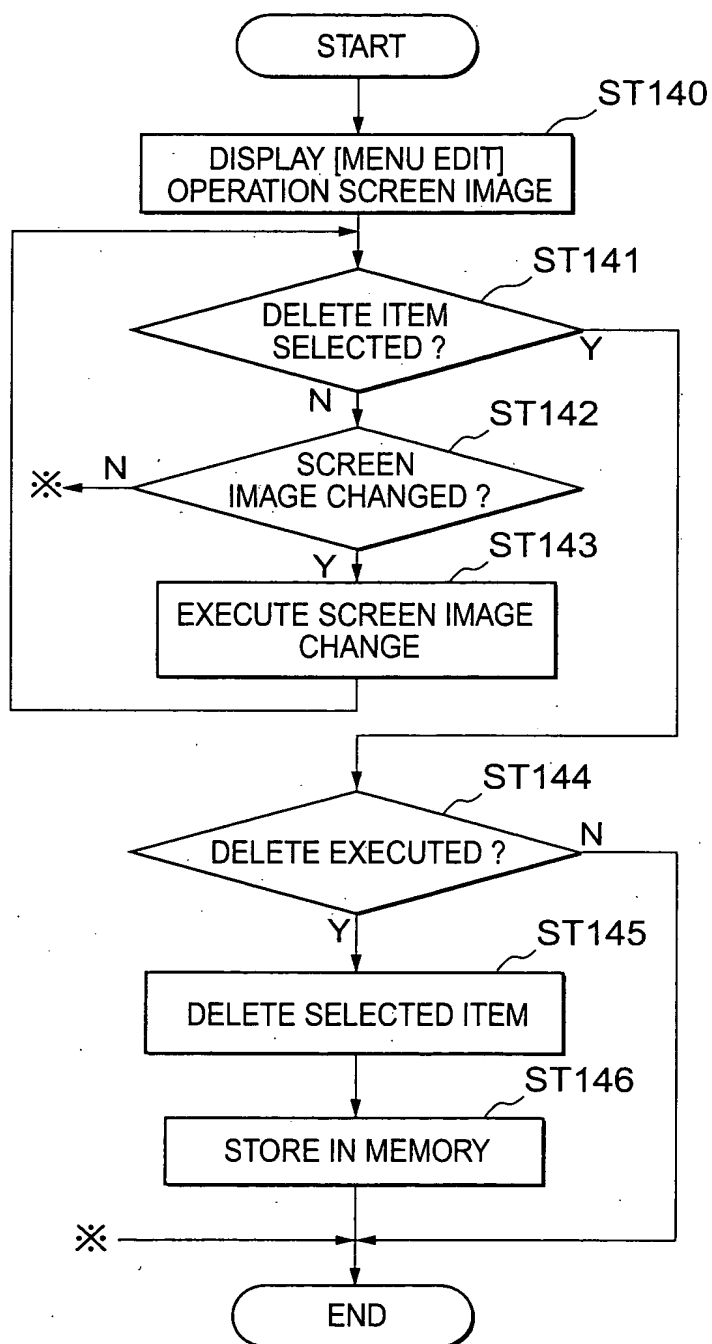

6/25

FIG. 8

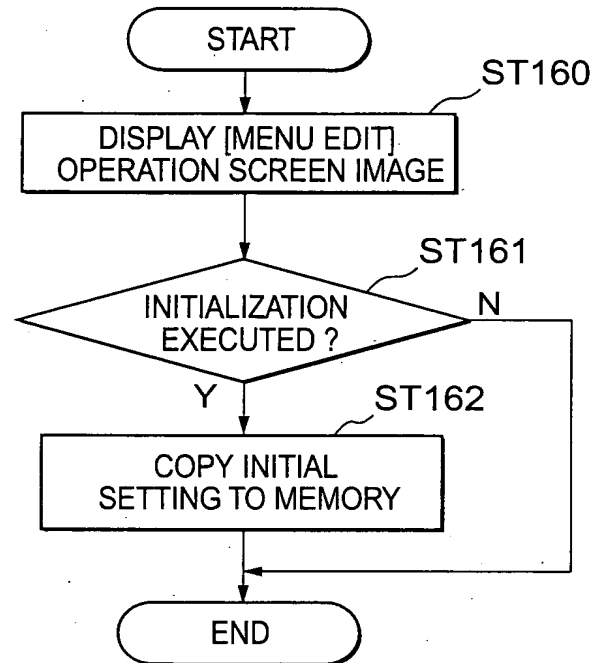

7/25

FIG. 9

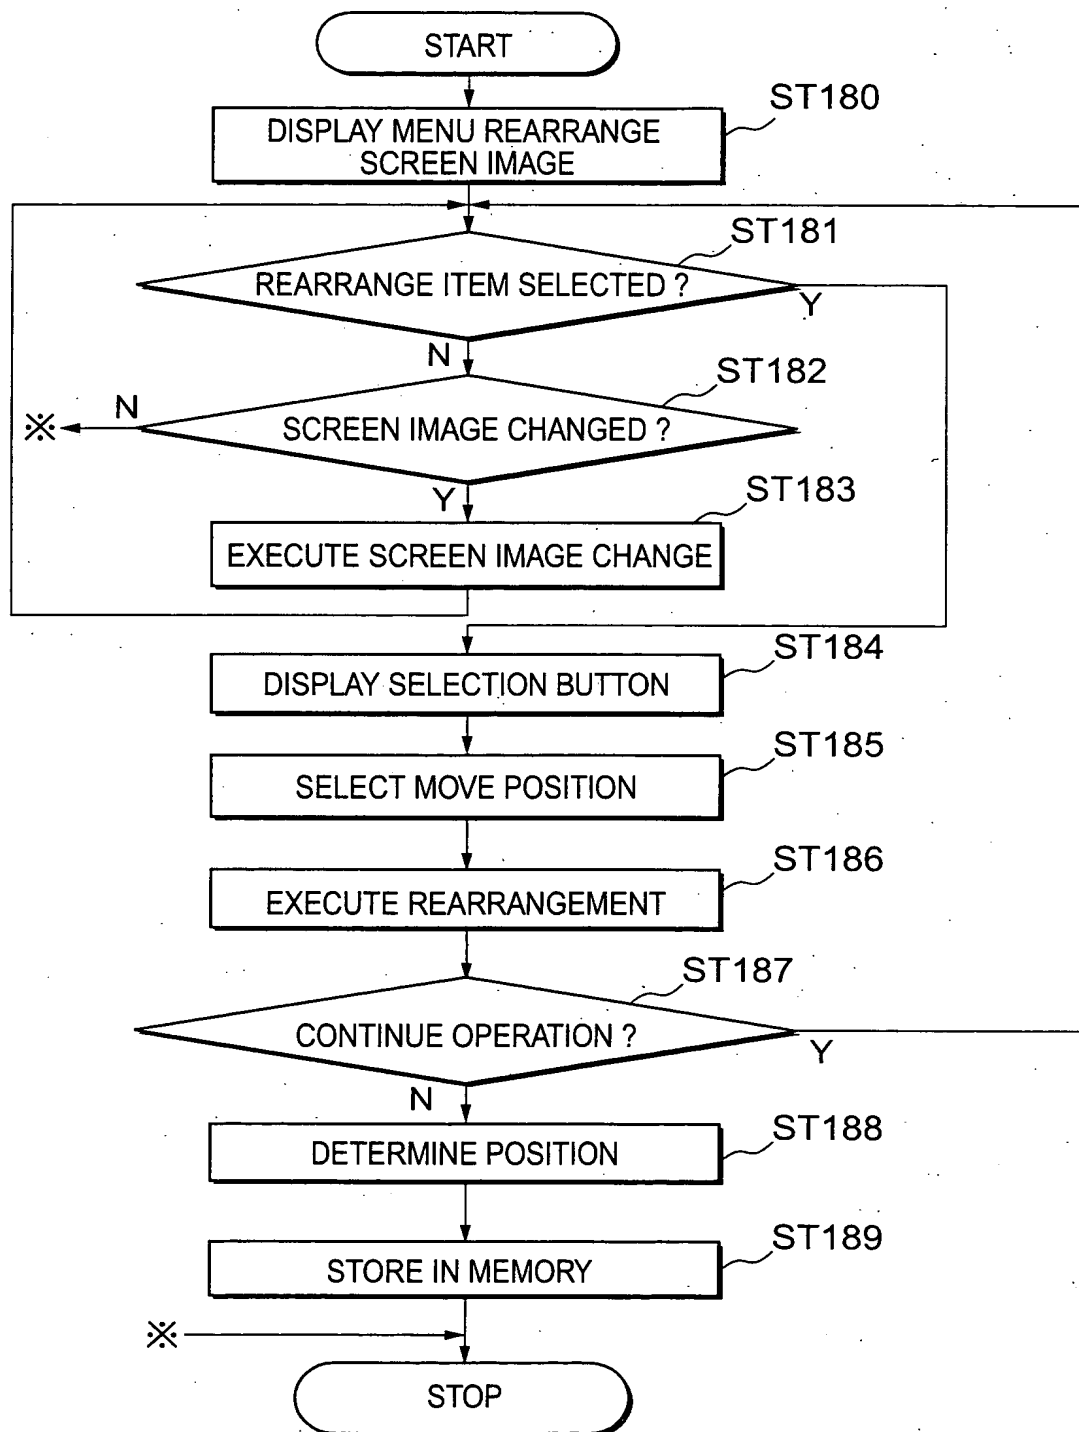


FIG. 10A

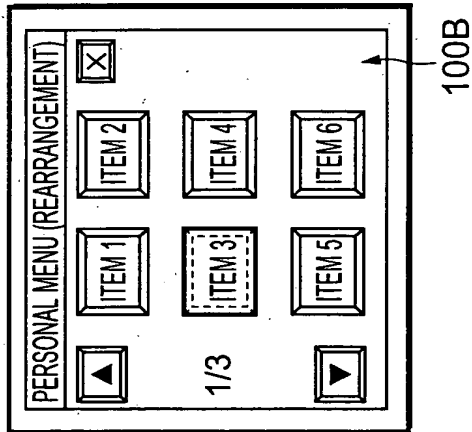


FIG. 10B

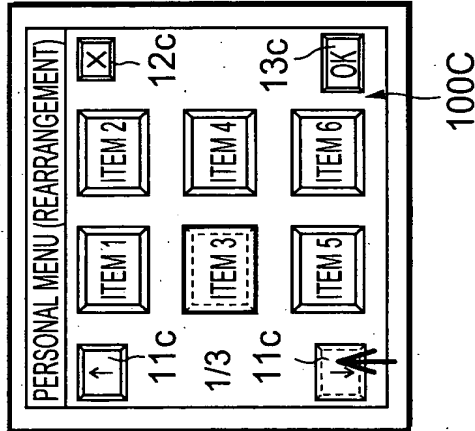


FIG. 10C

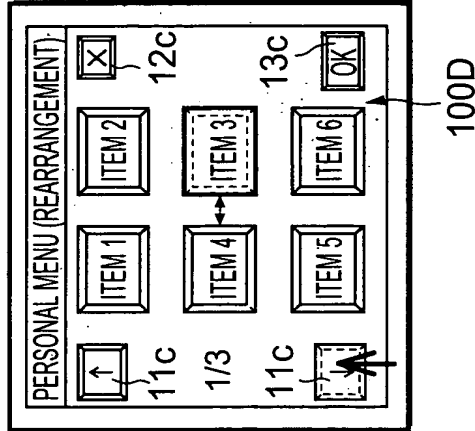


FIG. 10D


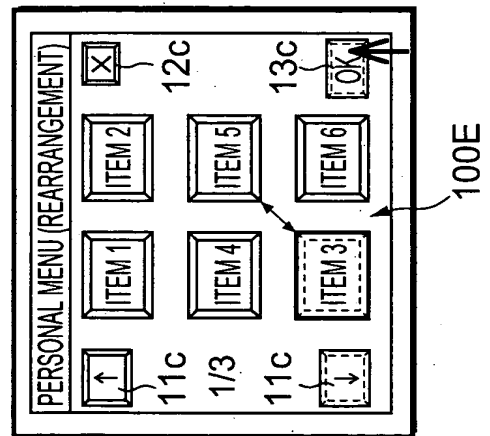



FIG. 10E



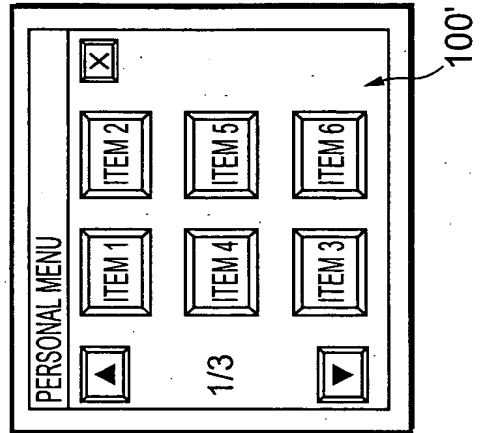


9/25

FIG. 11

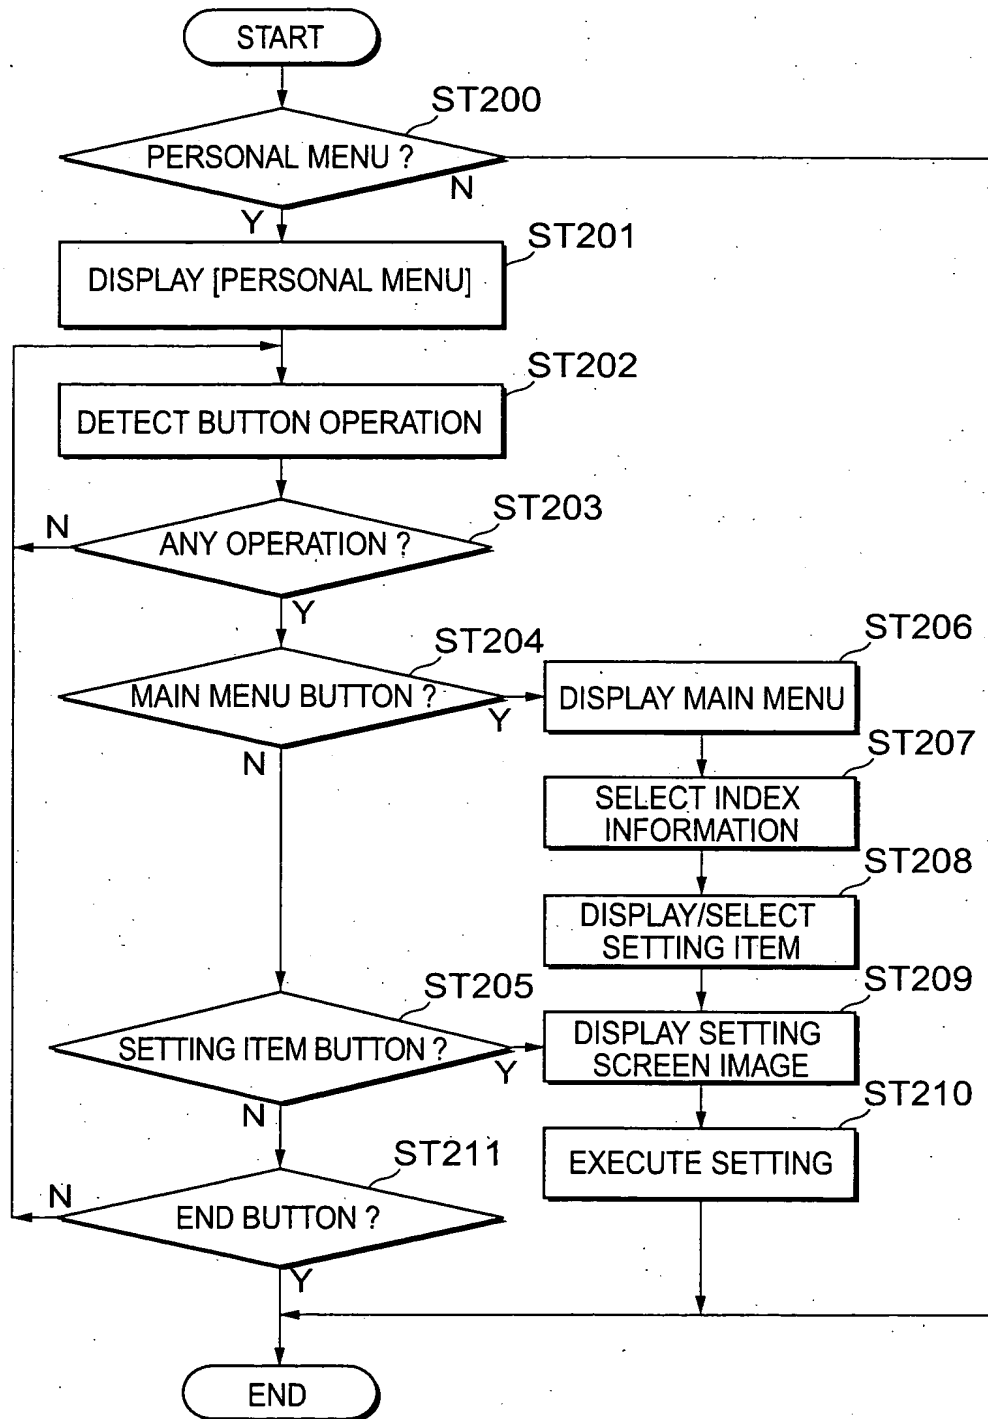


10/25

FIG. 12

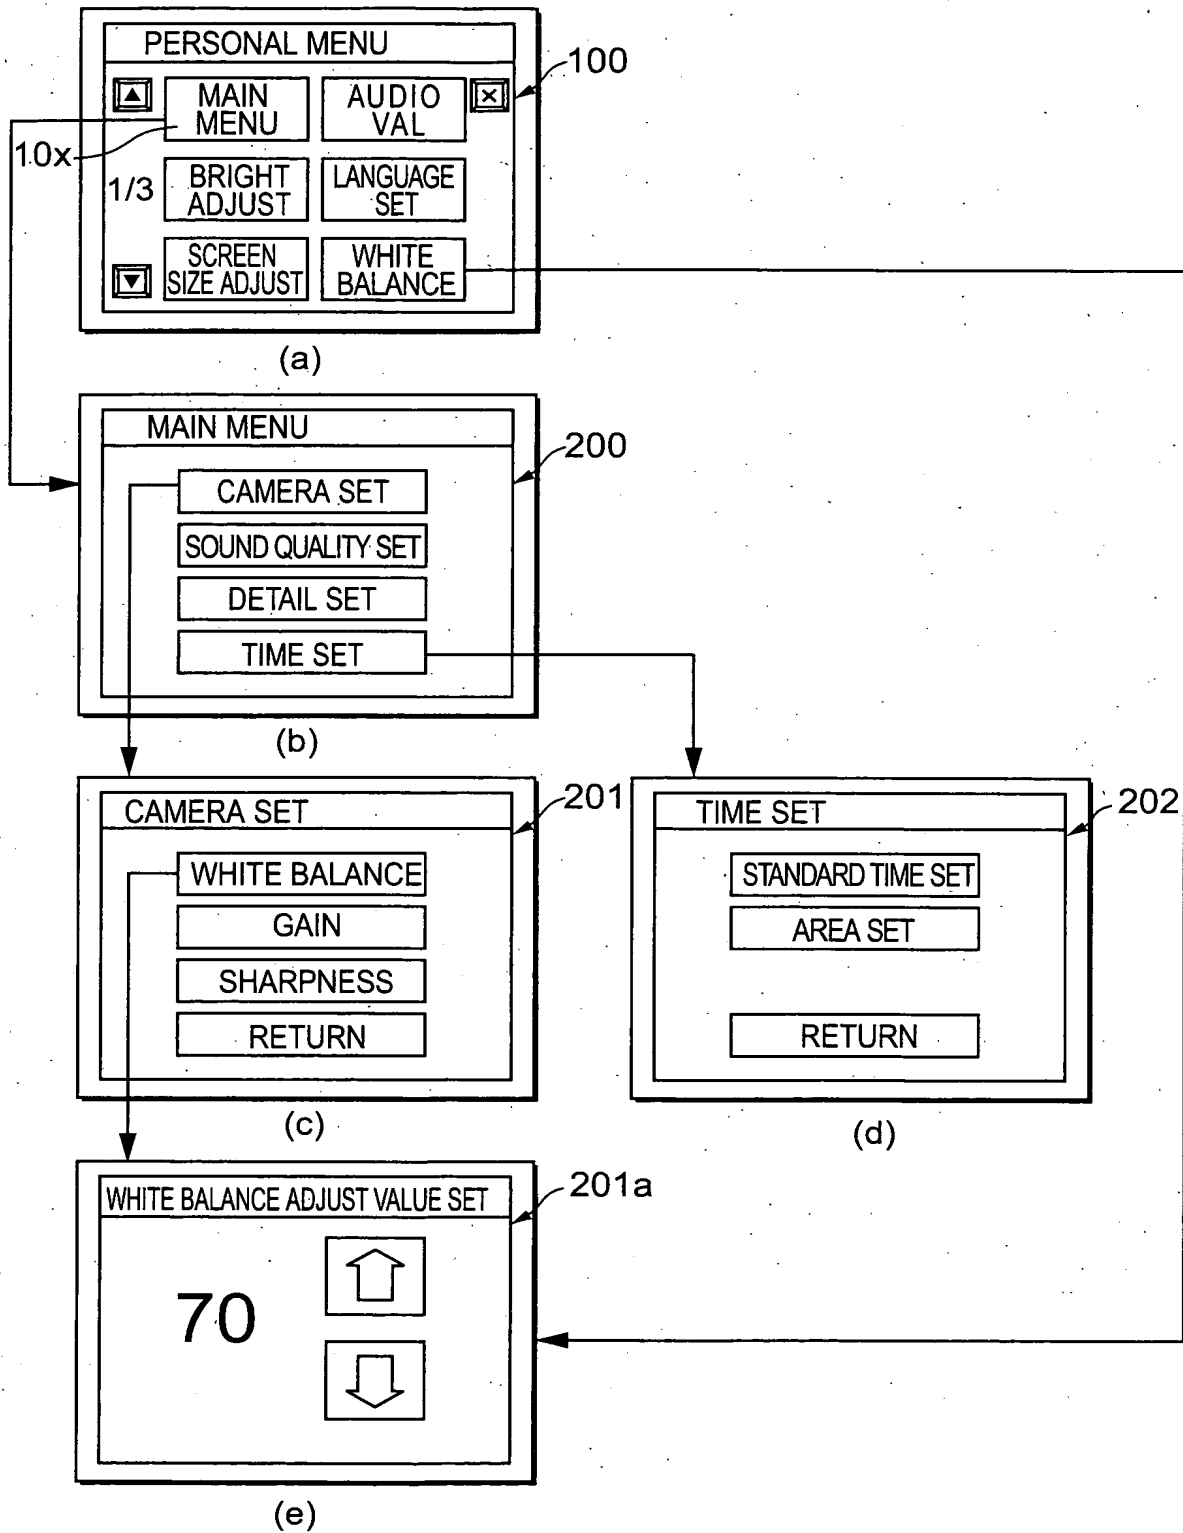

11/25

FIG. 13

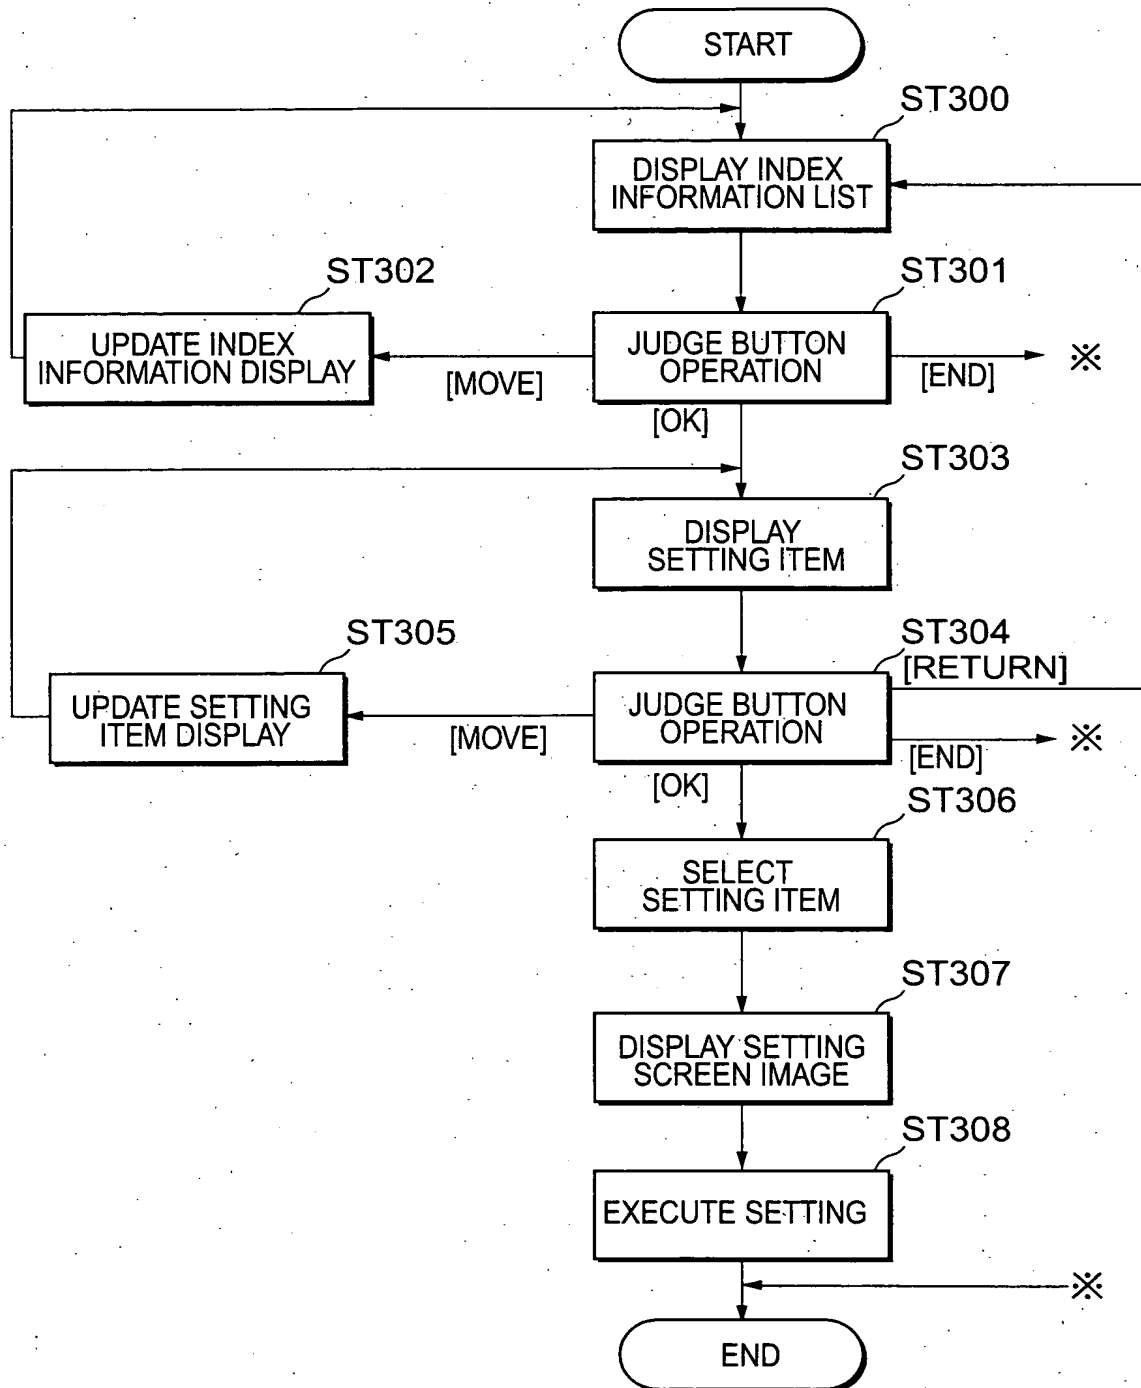

12/25

FIG. 14A

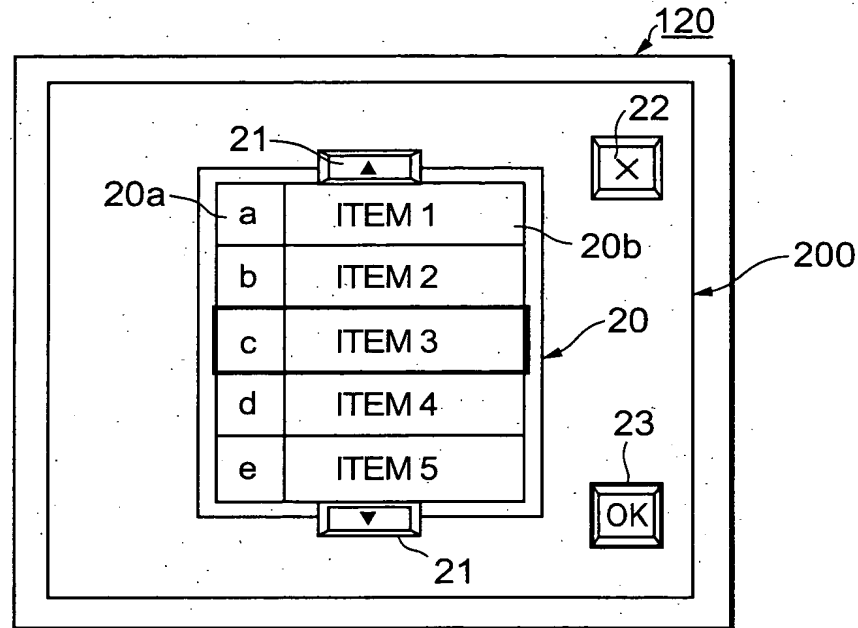


FIG. 14B

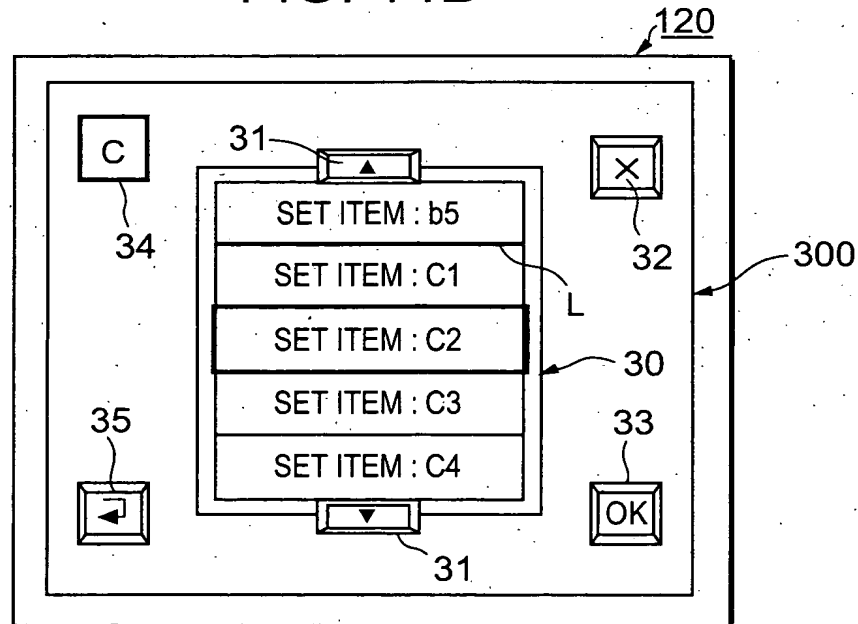


FIG. 15A




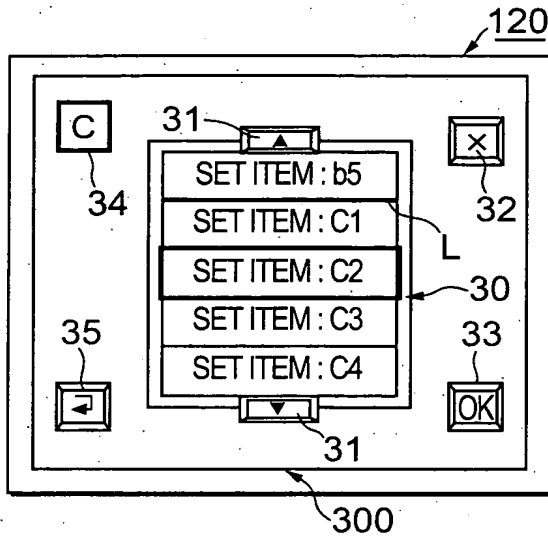


FIG. 15B

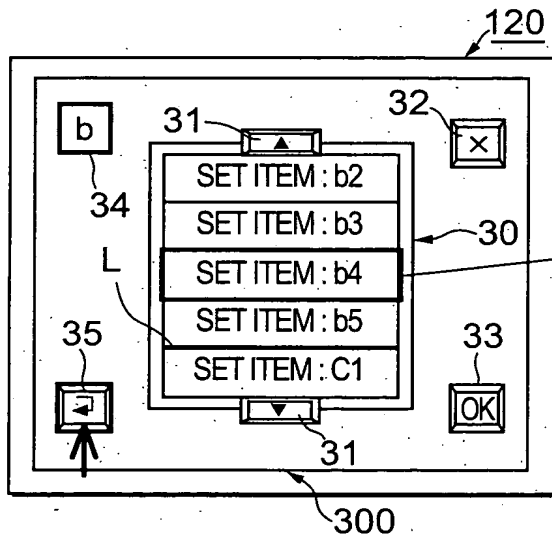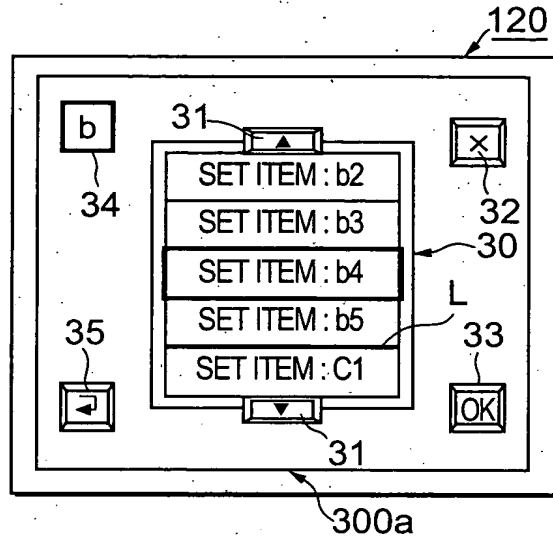

(a)

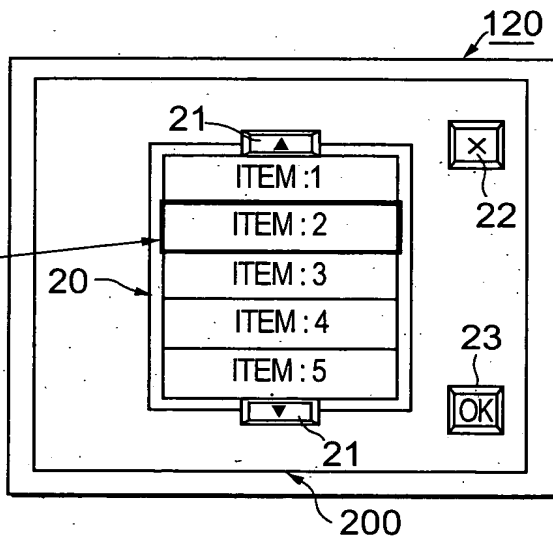

(b)

FIG. 16

14/25

FIG. 17A

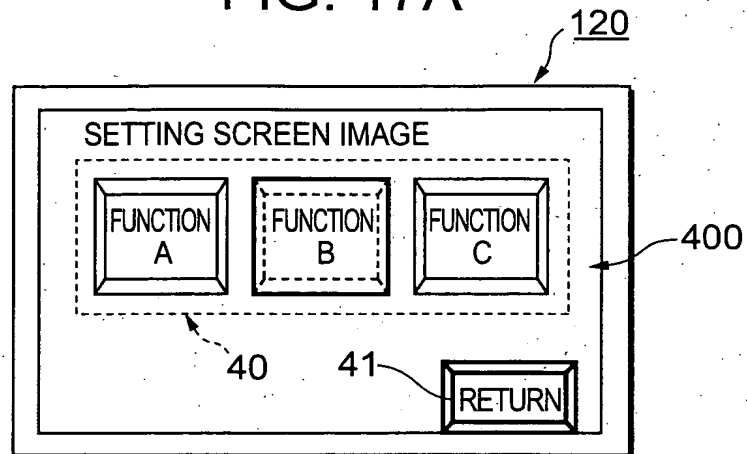


FIG. 17B

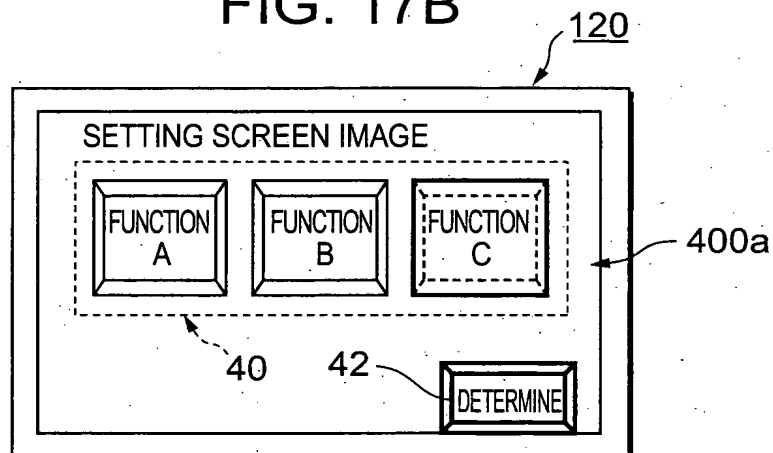


FIG. 17C

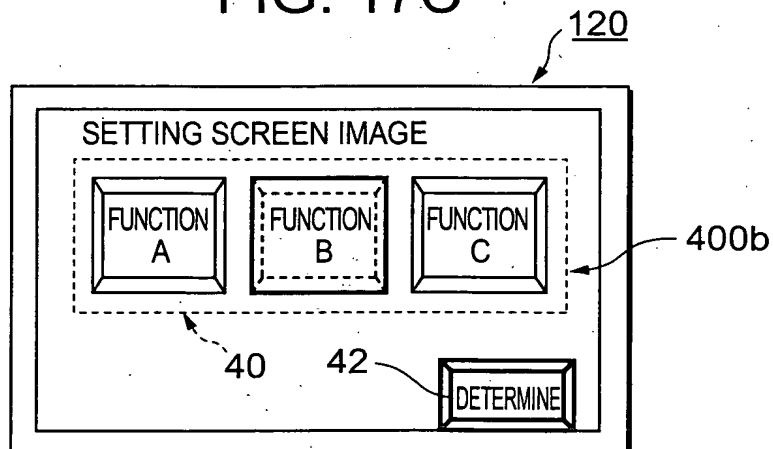


FIG. 18


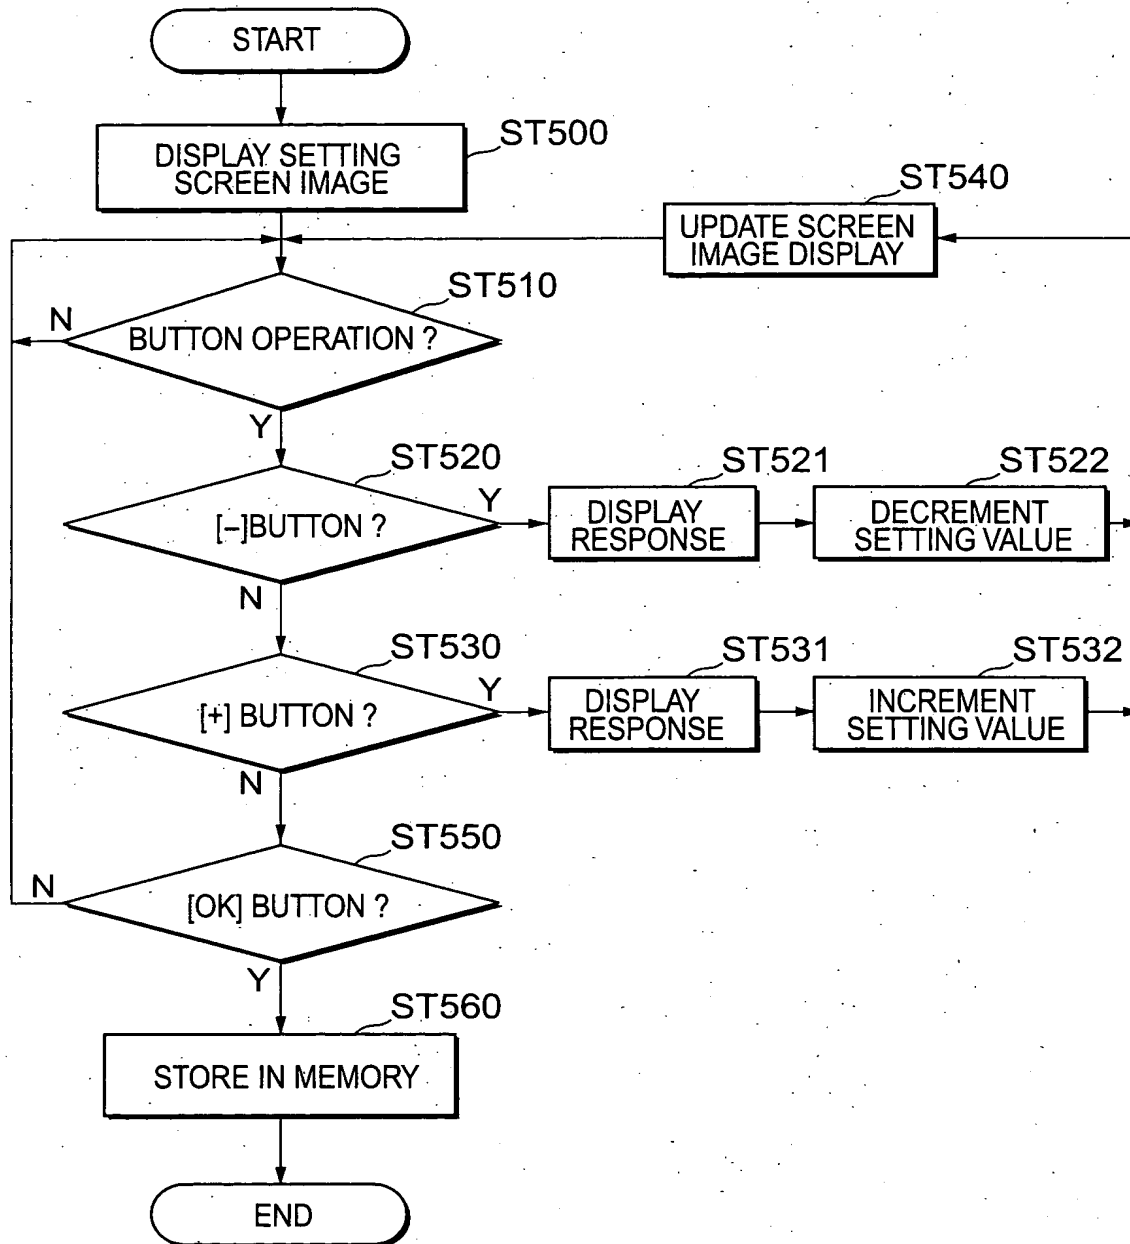


FIG. 19



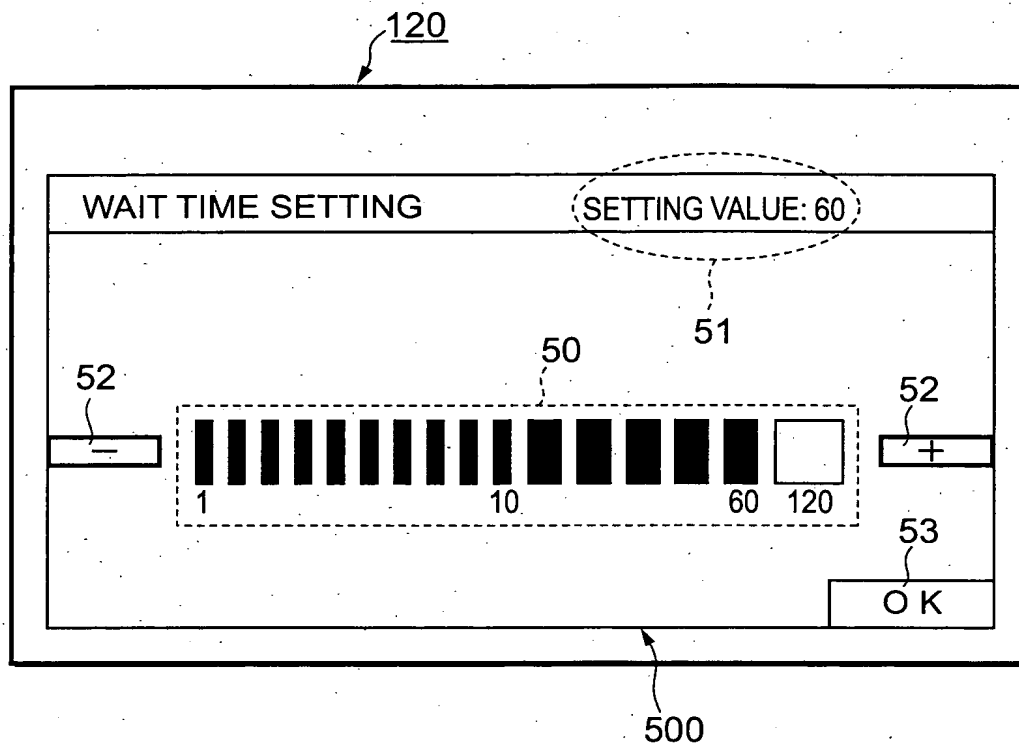

17/25

FIG. 20

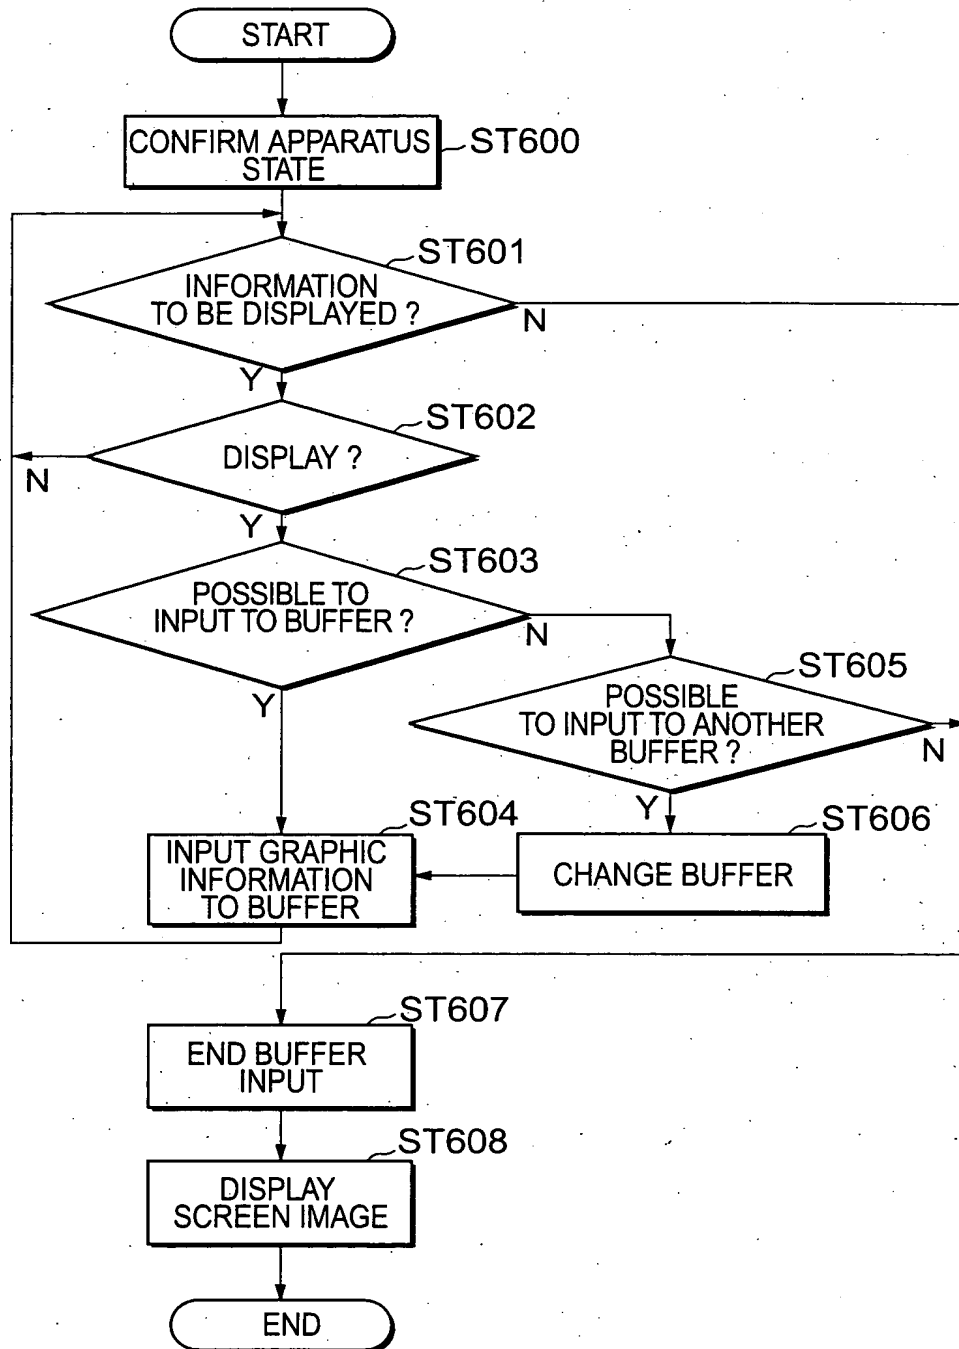


FIG. 21A

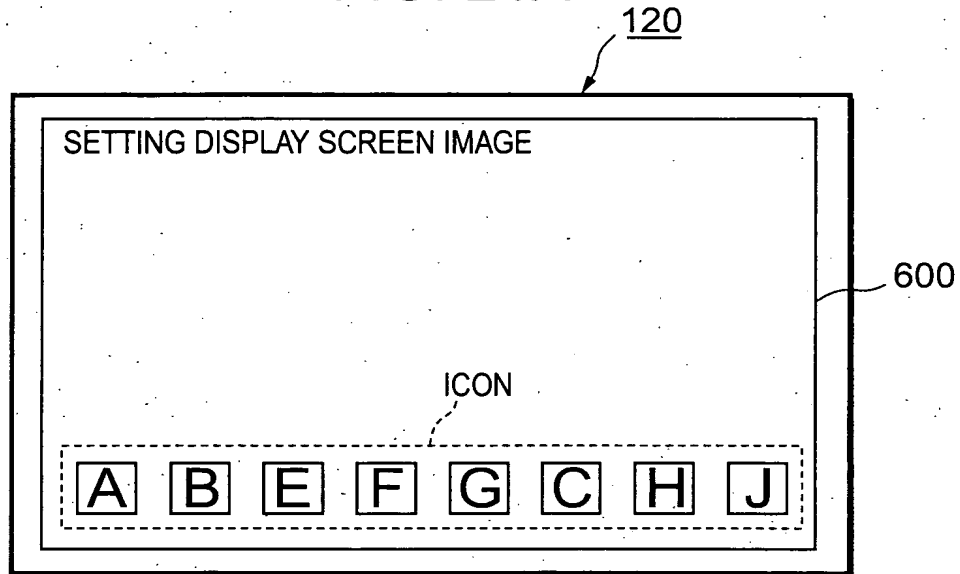


FIG. 21B


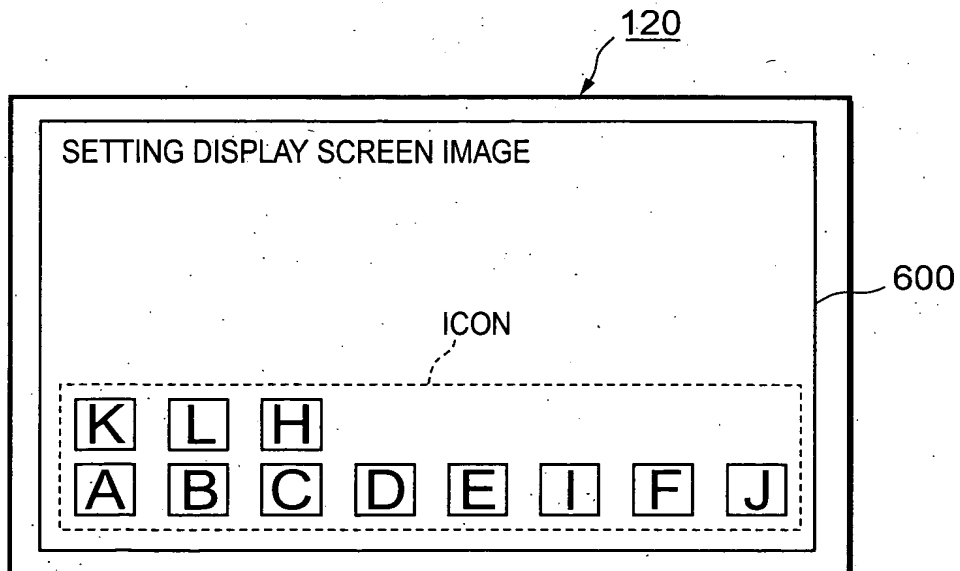


FIG. 22

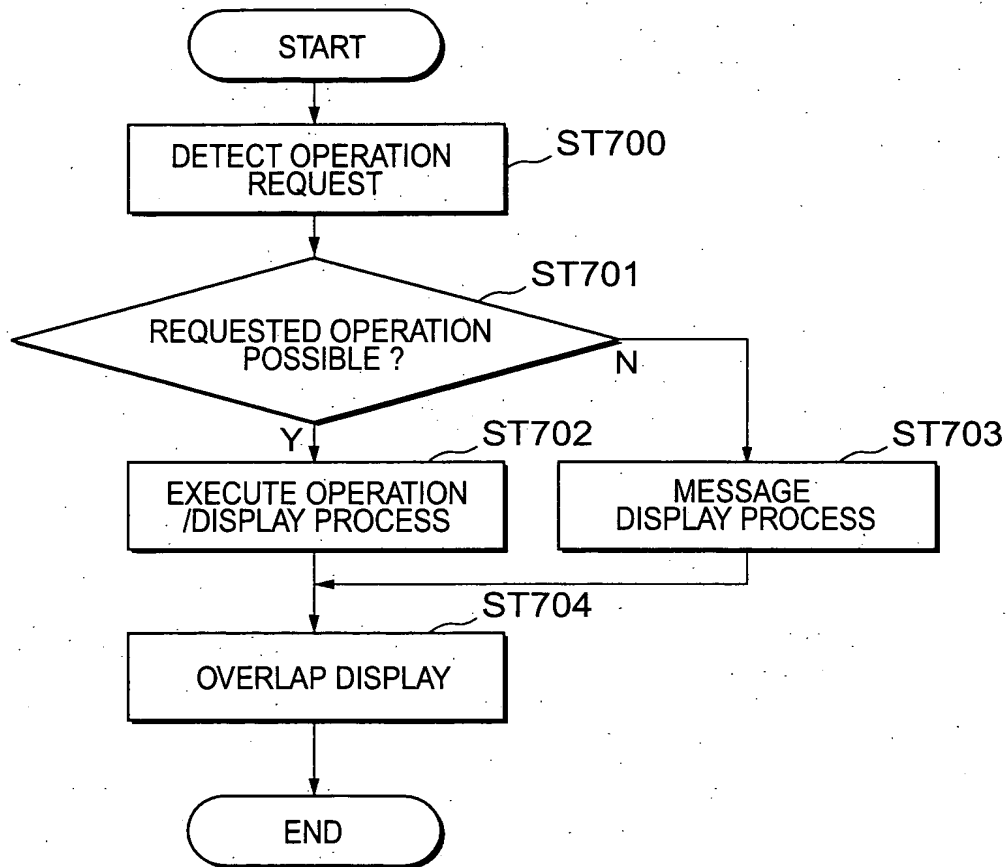

20/25

FIG. 23A

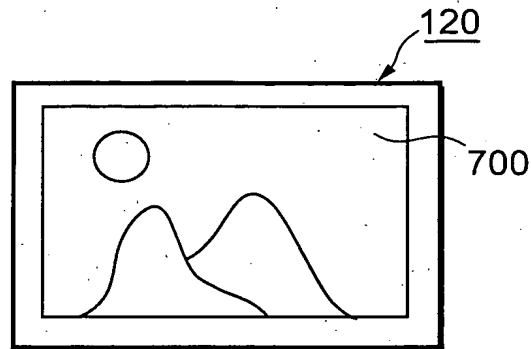


FIG. 23B

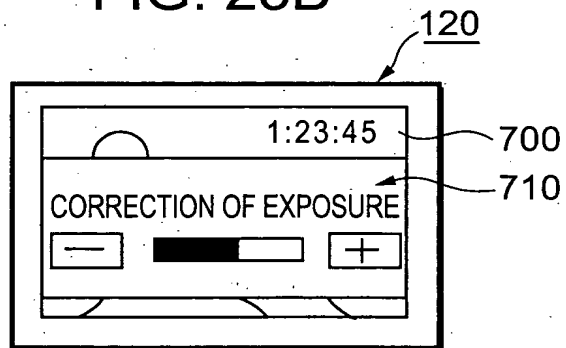


FIG. 23C

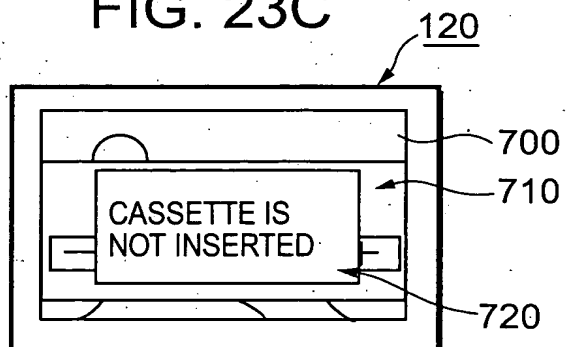


FIG. 24A

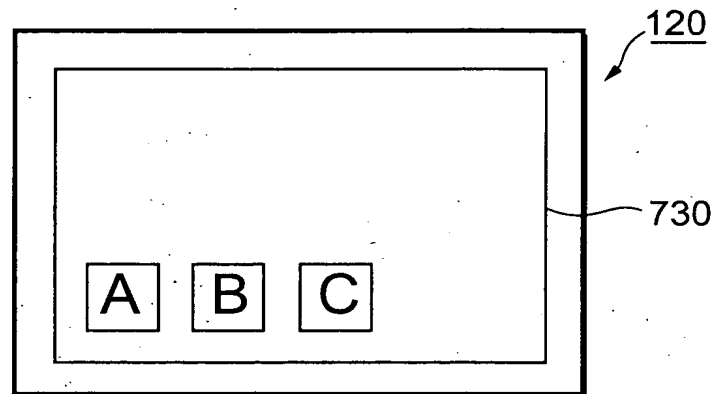


FIG. 24B


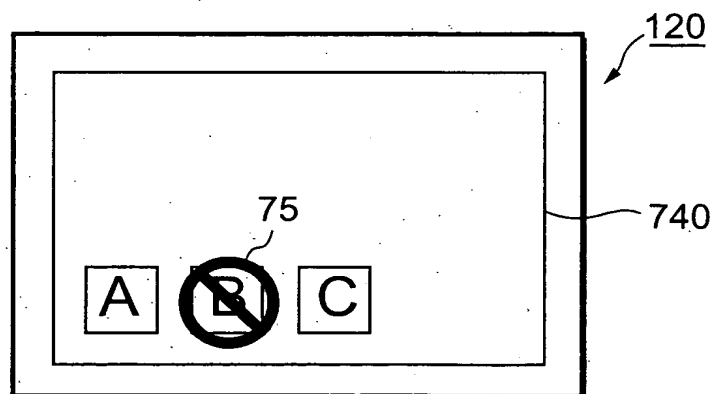


FIG. 25

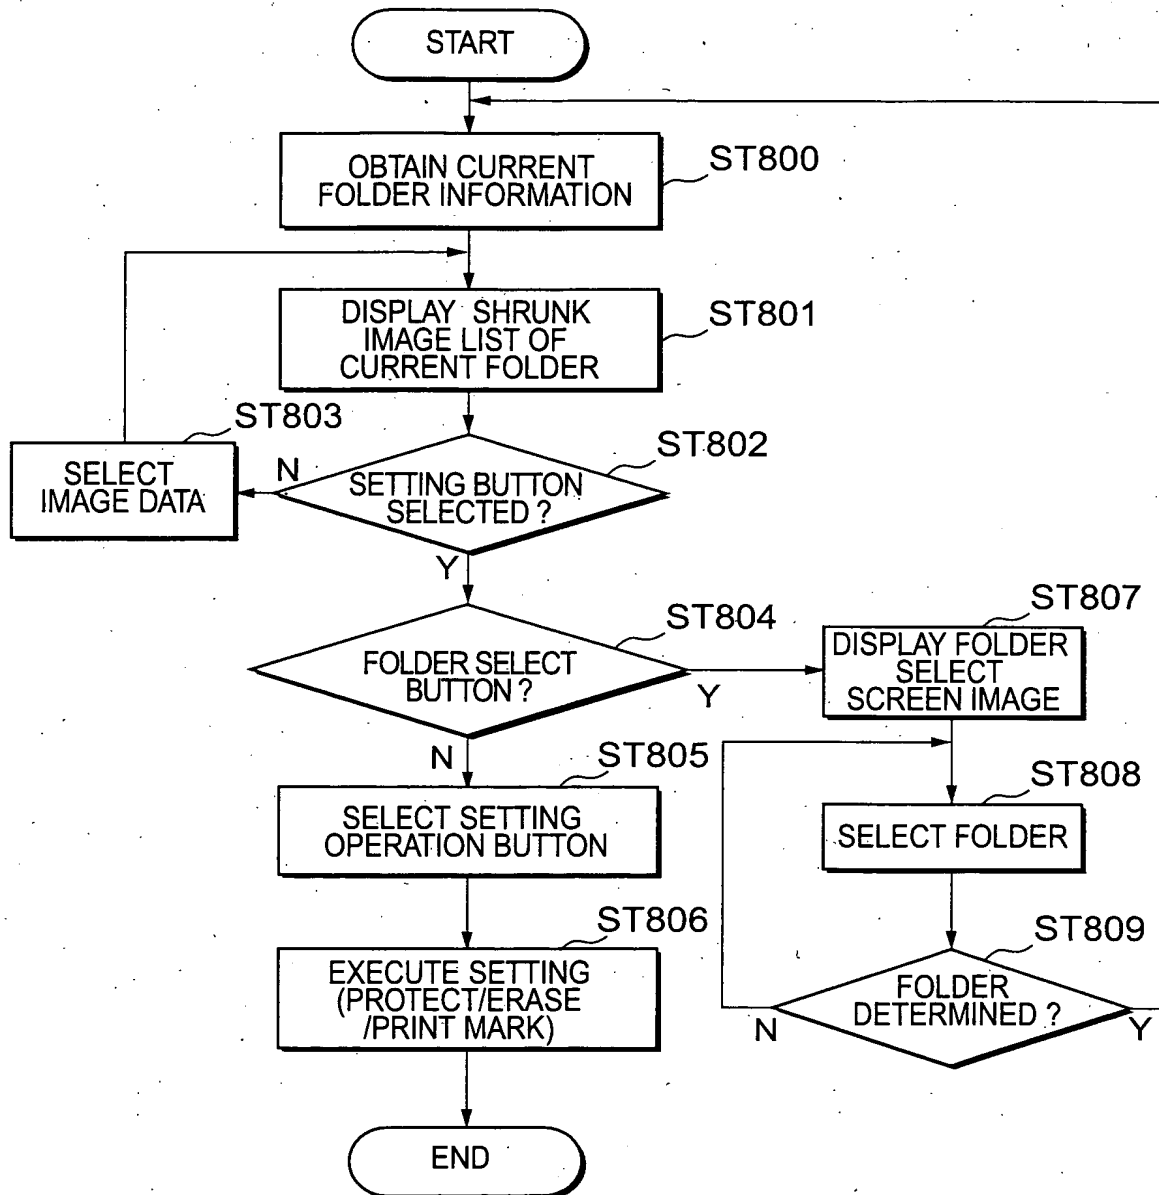

23/25

FIG. 26

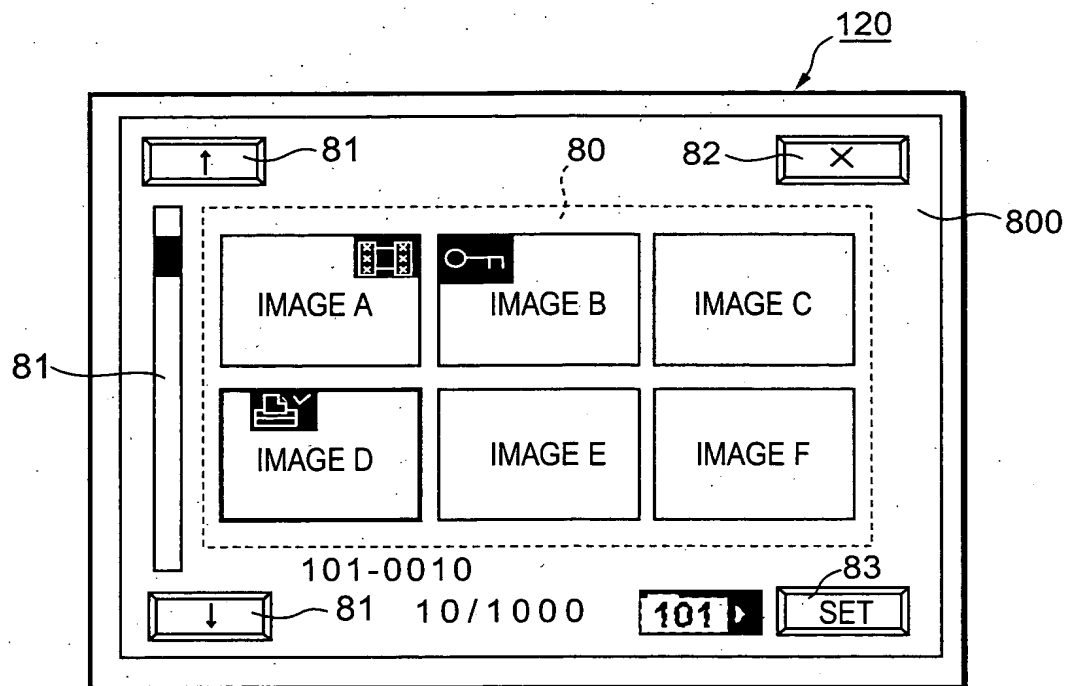


FIG. 27

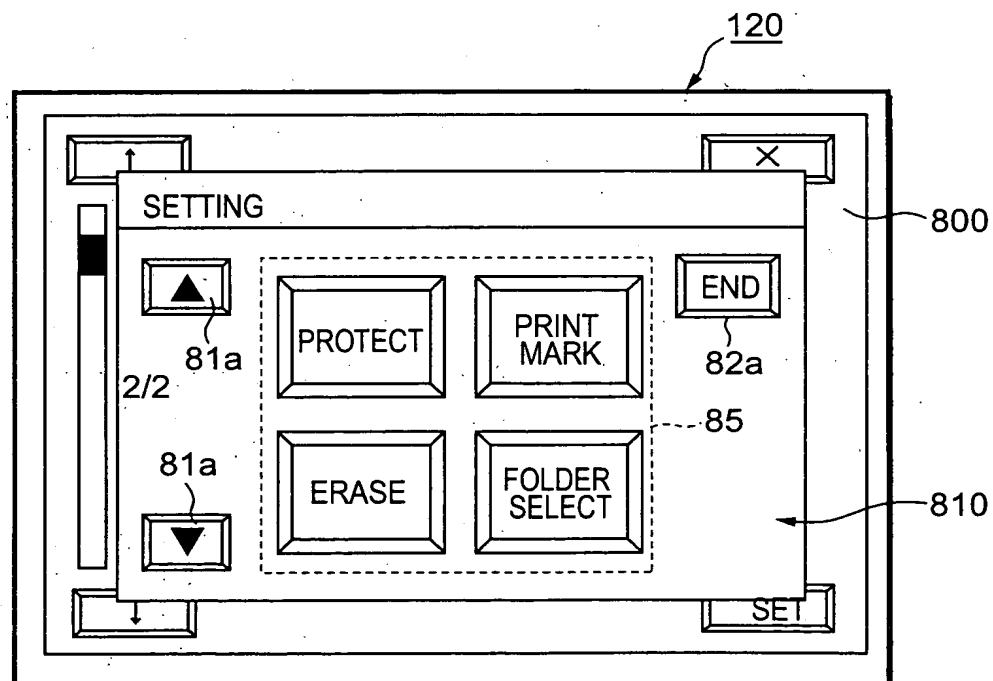


FIG. 28

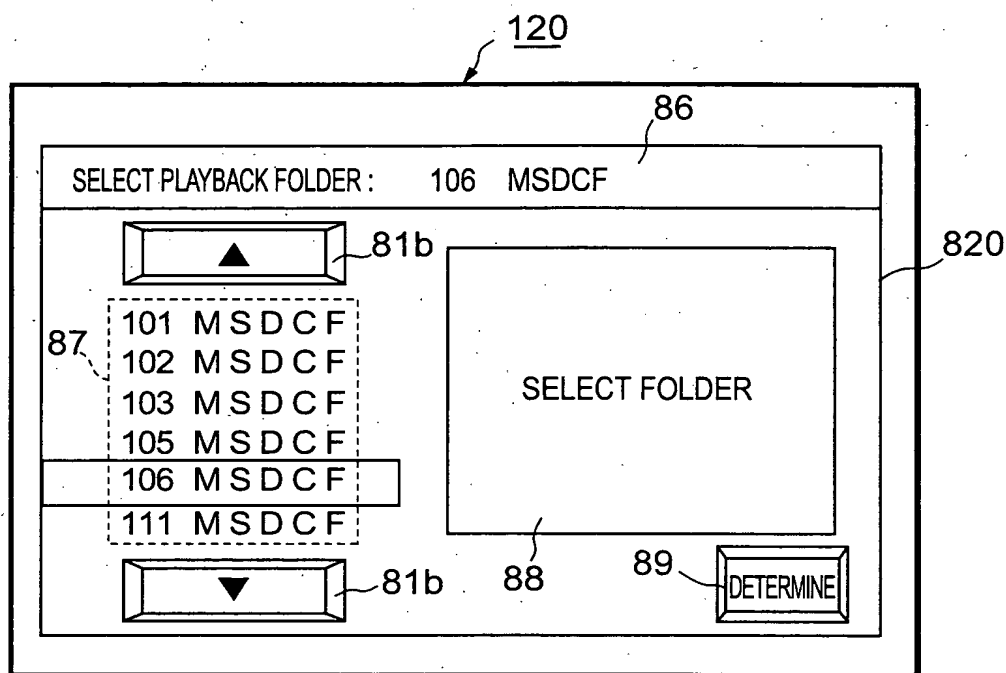






FIG. 29A

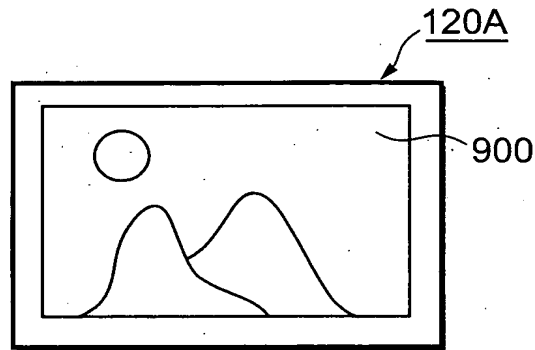


FIG. 29B

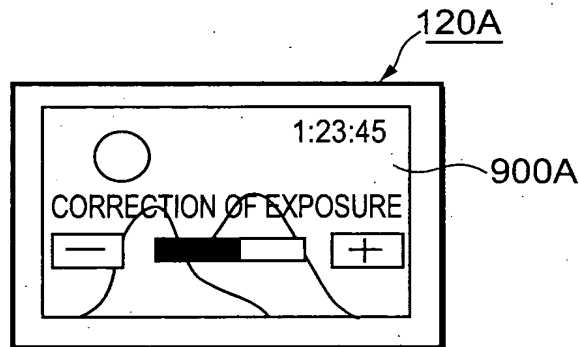


FIG. 29C

